

This Page Is Inserted by IFW Operations
and is not a part of the Official Record

BEST AVAILABLE IMAGES

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images may include (but are not limited to):

- BLACK BORDERS
- TEXT CUT OFF AT TOP, BOTTOM OR SIDES
- FADED TEXT
- ILLEGIBLE TEXT
- SKEWED/SLANTED IMAGES
- COLORED PHOTOS
- BLACK OR VERY BLACK AND WHITE DARK PHOTOS
- GRAY SCALE DOCUMENTS

IMAGES ARE BEST AVAILABLE COPY.

**As rescanning documents *will not* correct images,
please do not report the images to the
Image Problem Mailbox.**

ULTRASOUND ENHANCED CENTRAL VENOUS CATHETER

Peter Rule et al.

Appl. No.: Herewith Atty Docket: EKOS.095A

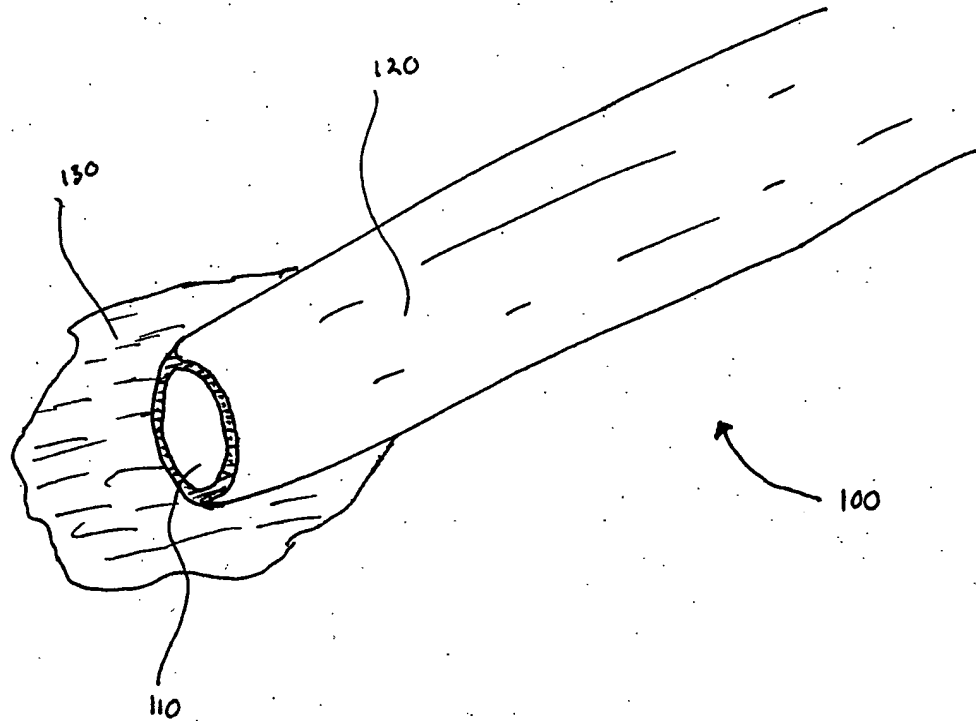


figure
one

ULTRASOUND ENHANCED CENTRAL VENOUS CATHETER

Peter Rule et al.

Appl. No.: Herewith Atty Docket: EKOS.095A

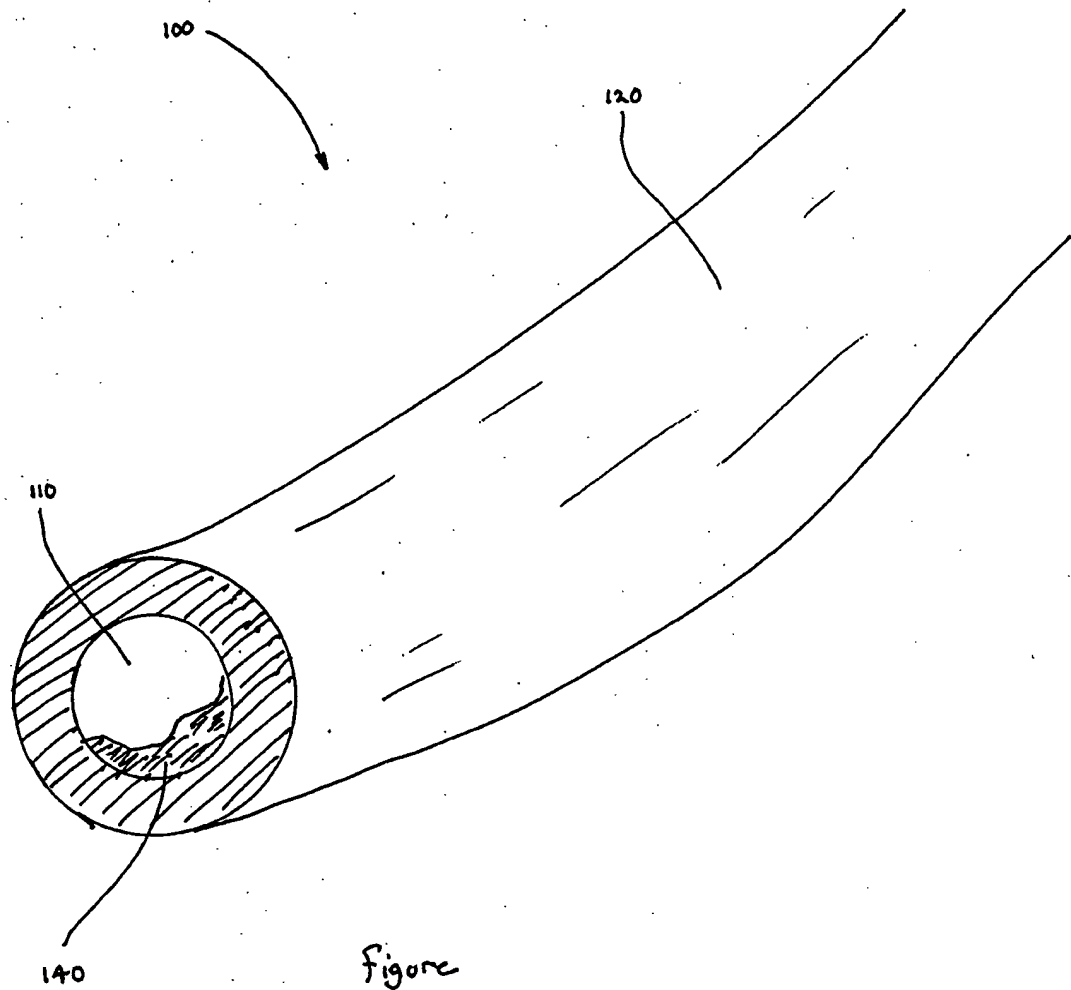




Figure
two

ULTRASOUND ENHANCED CENTRAL VENOUS CATHETER

Peter Rule et al.

Appl. No.: Herewith

Atty Docket: EKOS.095A

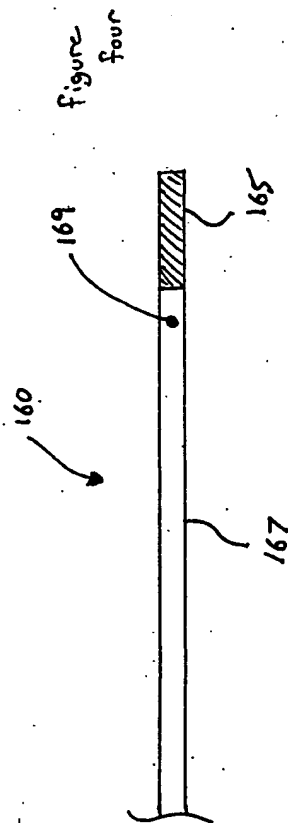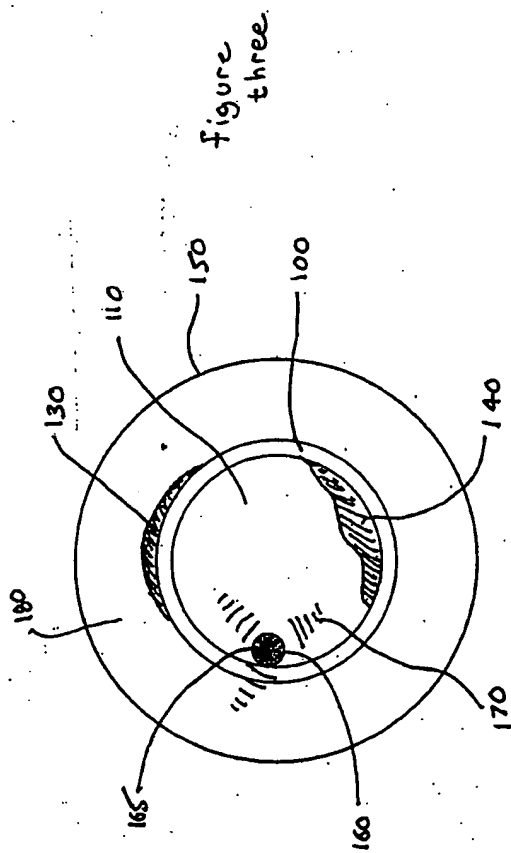


ULTRASOUND ENHANCED CENTRAL VENOUS CATHETER

Peter Rule et al.

Appl. No.: Herewith


Atty Docket: EKOS.095A

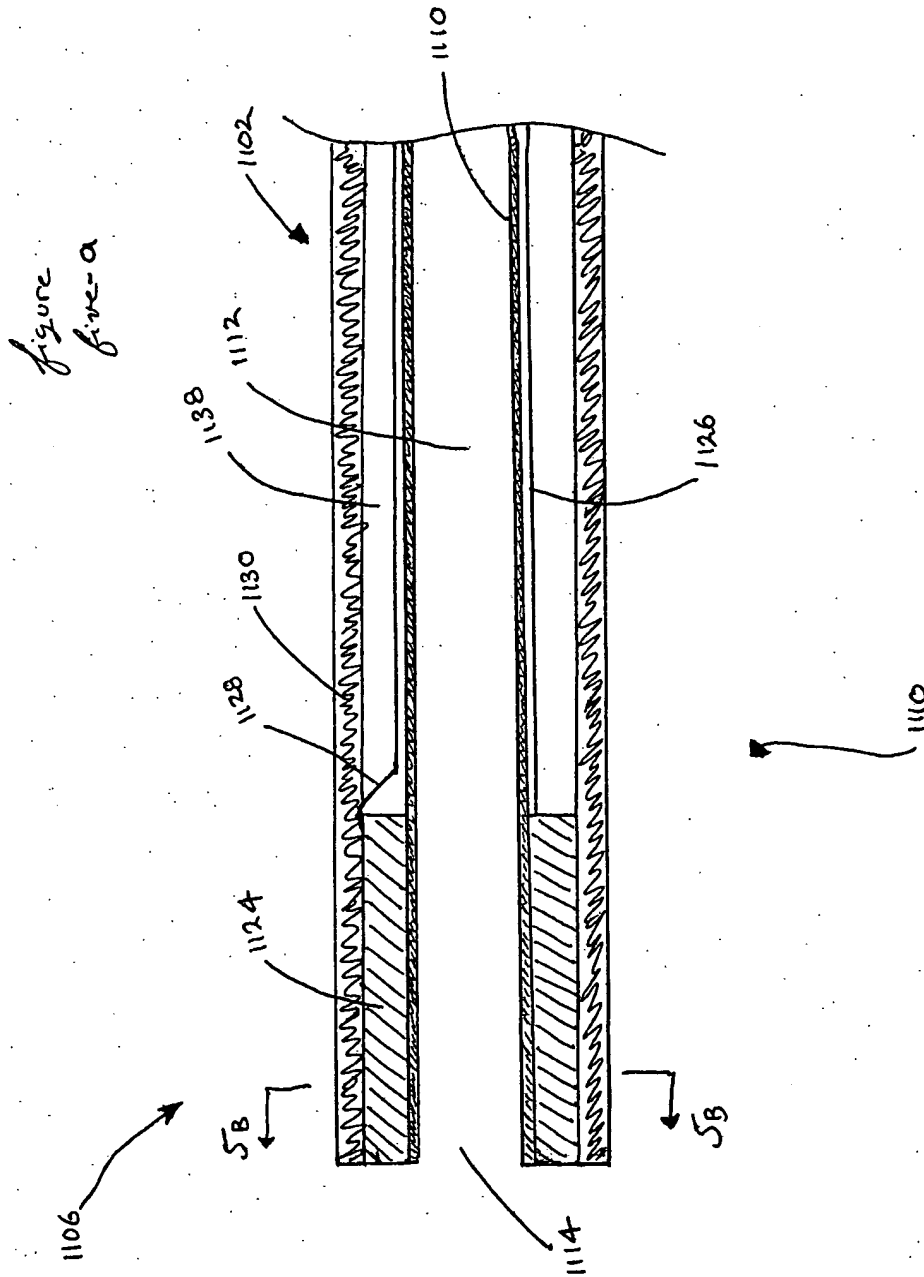

ULTRASOUND ENHANCED CENTRAL VENOUS CATHETER

Peter Rule et al.

Appl. No.: Herewith Atty Docket: EKOS.095A

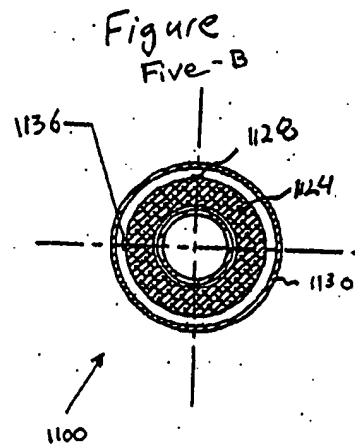

ULTRASOUND ENHANCED CENTRAL VENOUS CATHETER

Peter Rule et al.

Appl. No.: Herewith

Atty Docket: EKOS.095A

figure
six

